


Protocol for PicoWells In Chamber Slide


Innovative Biochips LLC
202 Industrial Blvd, Suite 703
Sugar Land, TX 77478, USA
+1 (832)538-1925
info@ibiochips.com
<https://ibiochips.com/>

Plasma Treatment

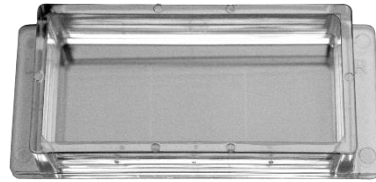


Take the lid off and put the *PicoWells In Chamber Slide* in a plasma cleaner. Treat the surface of picowells with plasma for 1-2 min to change the surface properties of PDMS picowells from being hydrophobic to hydrophilic.

Single-Cell Capture

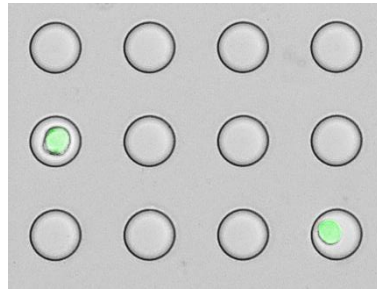


Pipette 1-2 mL of 30 mg/mL BSA/PBS solution into each well; wash away unabsorbed BSA after 1 h of incubation; add cell suspension (10^5 /mL); settle down for 10 min (~10% picowells will have single cells); wash away uncaptured cells.

Single-Bead Capture

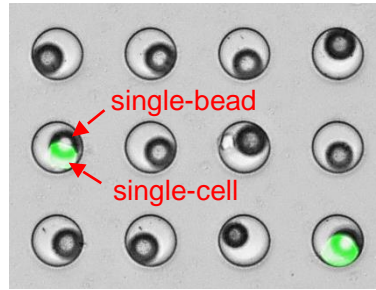

Place a Disk Magnet at the bottom of the picowells. Add the barcoded magnetic bead suspension ($\geq 10^6$ /mL) and settle down for 10 min to allow most picowells to capture single beads. Gently wash away the uncaptured beads.

Single-Cell Lysis

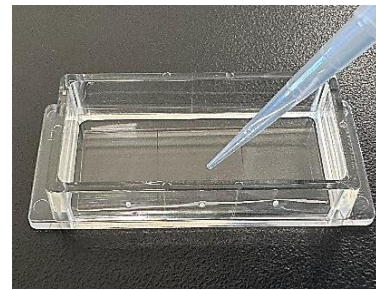

Add cold cell lysis buffer onto the surface of picowells; incubate for 10 min; add fresh lysis buffer (optional). The Disk Magnet at the bottom will increase the stability of magnetic beads within the picowells.

Beads Collection



Remove the Disk Magnet. Place a Cylinder Magnet on the surface of picowells, and move the Cylinder Magnet across the entire surface of picowells to collect the magnetic beads with captured mRNA.

Beads Transfer



Place a PCR tube containing PBS on top of a strong Cube Magnet. Insert the Cylinder Magnet containing magnetic beads with captured mRNA into the PBS; strongly stir up and down to transfer beads to the PCR tube.

Applications

- Single-Cell/Bead Isolation
- Single-Cell/Bead Imaging
- Single-Cell RNA-Sequencing

The Disk Magnet, Cylinder Magnet, and Cube Magnet need to be ordered separately.